





Molecular Imaging Products Company

A Division of Summit Anesthesia Support
Anesthesia Technologies


MAPLESON D – AS-01-0500-07

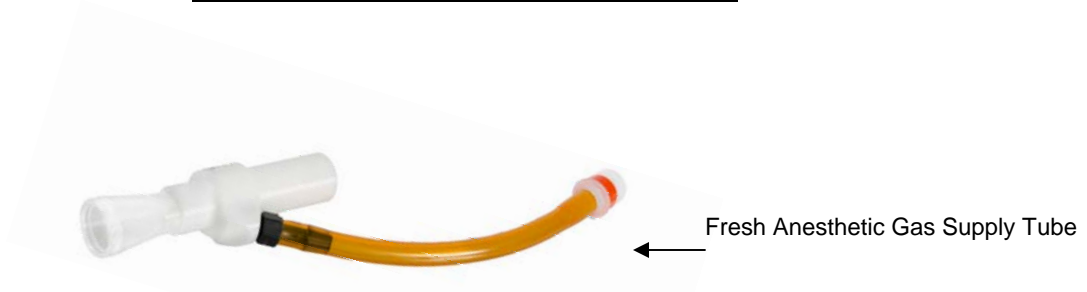


Use the above configurations with the Dual Diverter Manifold – AS-01-0529-01
Or the Dual Diverter Valve System – AS-01-0528

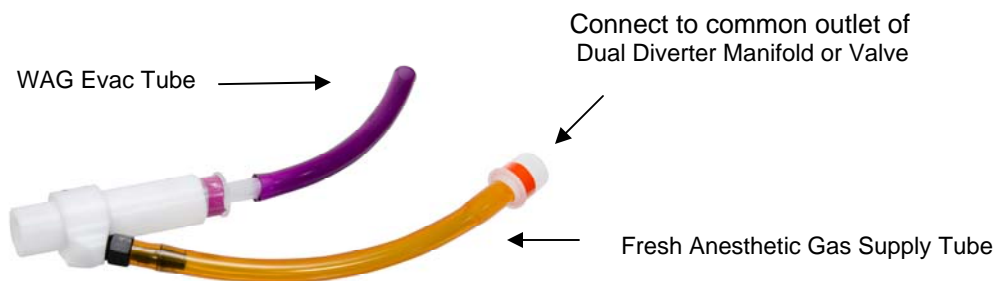


Use the above configurations with the Dual Diverter Manifold – AS-01-0529-01
Or the Dual Diverter Valve System – AS-01-0528

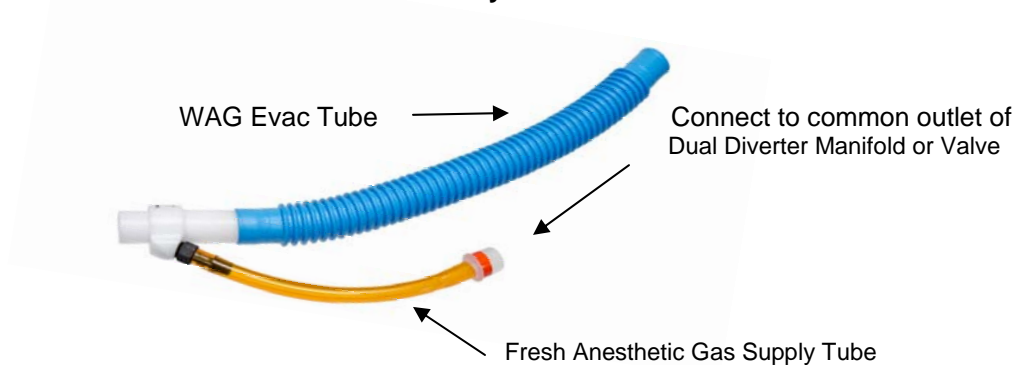


Use the above configurations with the Dual Diverter Manifold – AS-01-0529-01
Or the Dual Diverter Valve System – AS-01-0528

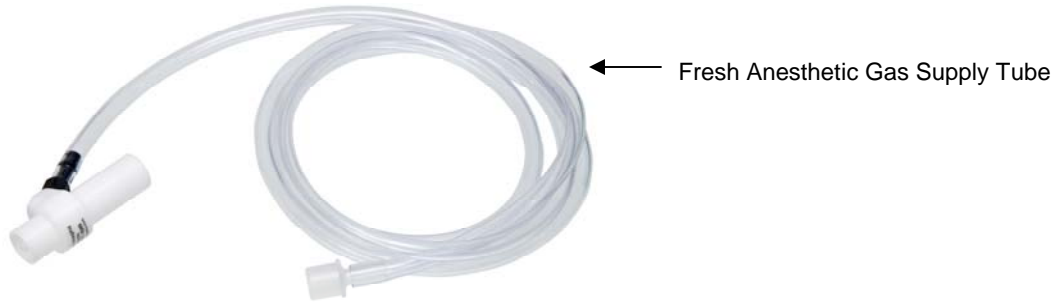

Use the above configuration when connecting directly to the vaporizer

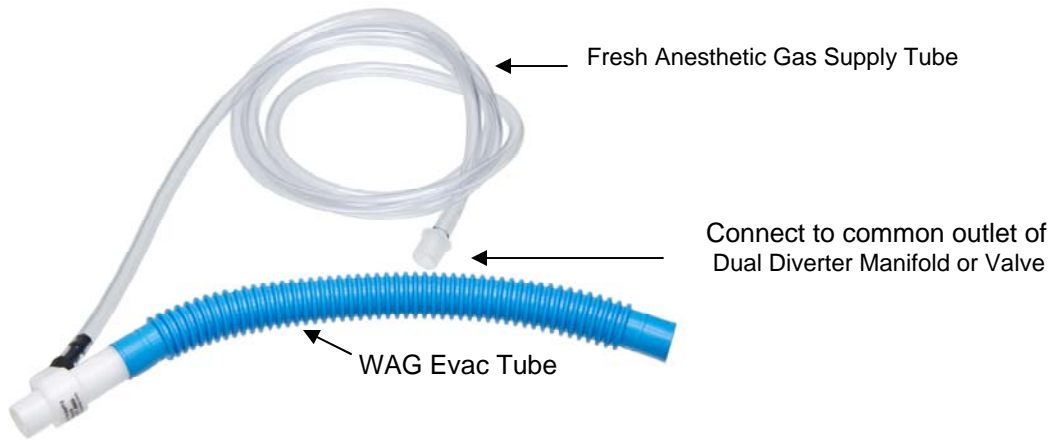

Use the above configuration when connecting directly to the vaporizer

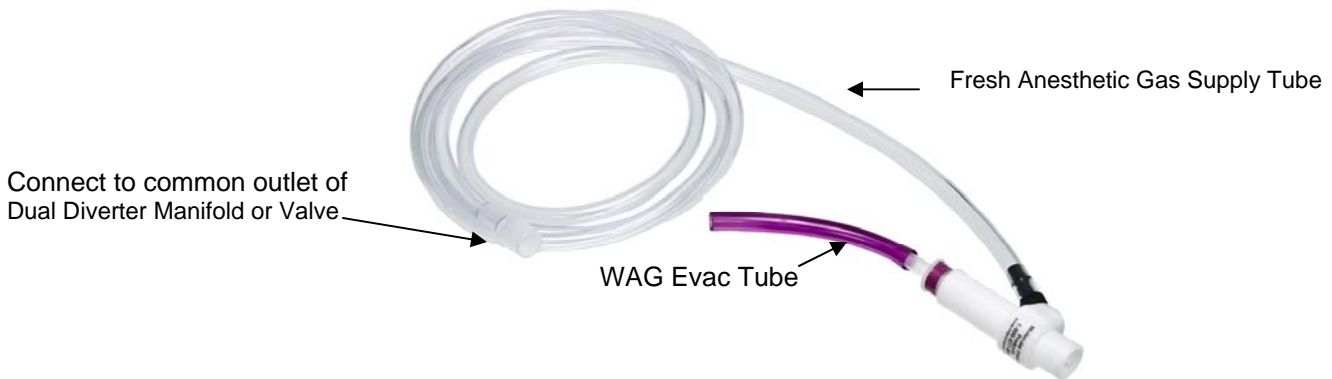

Use the above configuration when connecting directly to the vaporizer